

DETECT WITH CONFIDENCE

SHIGA TOXIN CHEK™

Provide complete and accurate results

- Direct detection of STEC toxins from primary fecal specimens
- Simultaneously detect Stx1 and Stx2
- Detect serogroups O157 and non-O157 (non-O157 is not easily detectable by culture)
- Shorter time to result than other ELISA assay or culture method



SHIGA TOXIN CHEK™

Product Order Information

Product Name	Cat. No.	Sample Type	Time to Result	Format
SHIGA TOXIN CHEK™	T30696	Fresh and frozen fecal sample (unpreserved), Cary Blair, C&S, broth (GN or MAC), plate culture (SMAC, CT-SMAC, CHROMagar® O157)	50 minutes, or 20 minutes (rapid)	Microplate ELISA


SHIGA TOXIN CHEK™

Specimen Preparation

Direct Fecal Method

Add to a test tube:


- 200 µL *Diluent* (3rd graduation)
- 50 µL (1st graduation) of specimen*
- Mix thoroughly.



*For specimens in transport media, use 100 µL *Diluent* and 100 µL Specimen (2nd graduation)


Broth Method

- A** Add 25 µL of specimen* to a tube containing 8mL of GN or 5mL of MacConkey Broth




*For specimens in transport media, use 100 µL Specimen

- B** Loosely cap the inoculated broth and incubate for 16-24 hours at 37°C ± 2°C. Examine the tube for growth. If no growth, do not proceed with testing.



- C** Add to a test tube:


- 200 µL *Diluent* (3rd graduation)
- 50 µL (1st graduation) of broth culture.
- Mix thoroughly.



Assay Protocol

- 1** Add to wells:
- 1 drop *Conjugate*
 - 100 µL (2nd graduation) of diluted specimen or diluted broth culture, or appropriate amount of controls

Incubate wells for 50 minutes at 37°C ± 2°C




Note: A 20-minute alternate expedited incubation step is possible if the specimen is incubated at 37°C with shaking.



- 2** Wash wells with diluted *Wash Buffer* 5 times. Slap inverted plate firmly on paper towels between each wash.



- 3** Add 2 drops of *Substrate* to all test wells. Incubate wells at room temperature for 10 minutes. Tap wells gently to mix during incubation.



- 4** Add 1 drop *Stop Solution*. Tap to mix. Wait 2 minutes before reading. Refer to the package insert for interpretation of results.

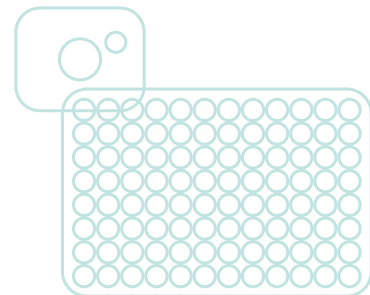

www.cdc.gov/ecoli
SHIGA TOXIN CHEK™ Package Insert

TECHLAB, Inc. is a leading developer and manufacturer of infectious disease diagnostics products worldwide. Since 1989, the company has offered a quality portfolio of diagnostic tests which now includes assays for *C. difficile*, *Campylobacter*, Shiga toxin producing *E. coli*, *H. pylori*, protozoan parasites, and biomarkers of intestinal inflammation.



© 2021 TECHLAB, Inc. All rights reserved.

SHIGA TOXIN CHEK, the TECHLAB Logo, and TECHLAB are trademarks of TECHLAB, Inc. All other trademarks referenced are trademarks of their respective owners. PN 842021178

Distributed by



T 01782 575180 | E info@unahealth.co.uk | W www.unahealth.co.uk
Unit 3, Fitzgerald Way, Scotia Road Business Park, Stoke-on-Trent, ST6 4HN

Developed and manufactured by



PROVEN DIAGNOSTIC PERFORMANCE